


ZONE		REV.	DESCRIPTION	DATE	APPROVED
All	0		INITIAL RELEASE	16MAR05	PC
All	1		GENERAL UPDATE	16MAR06	REB
All	2		GENERAL UPDATE	24APR22	DRS

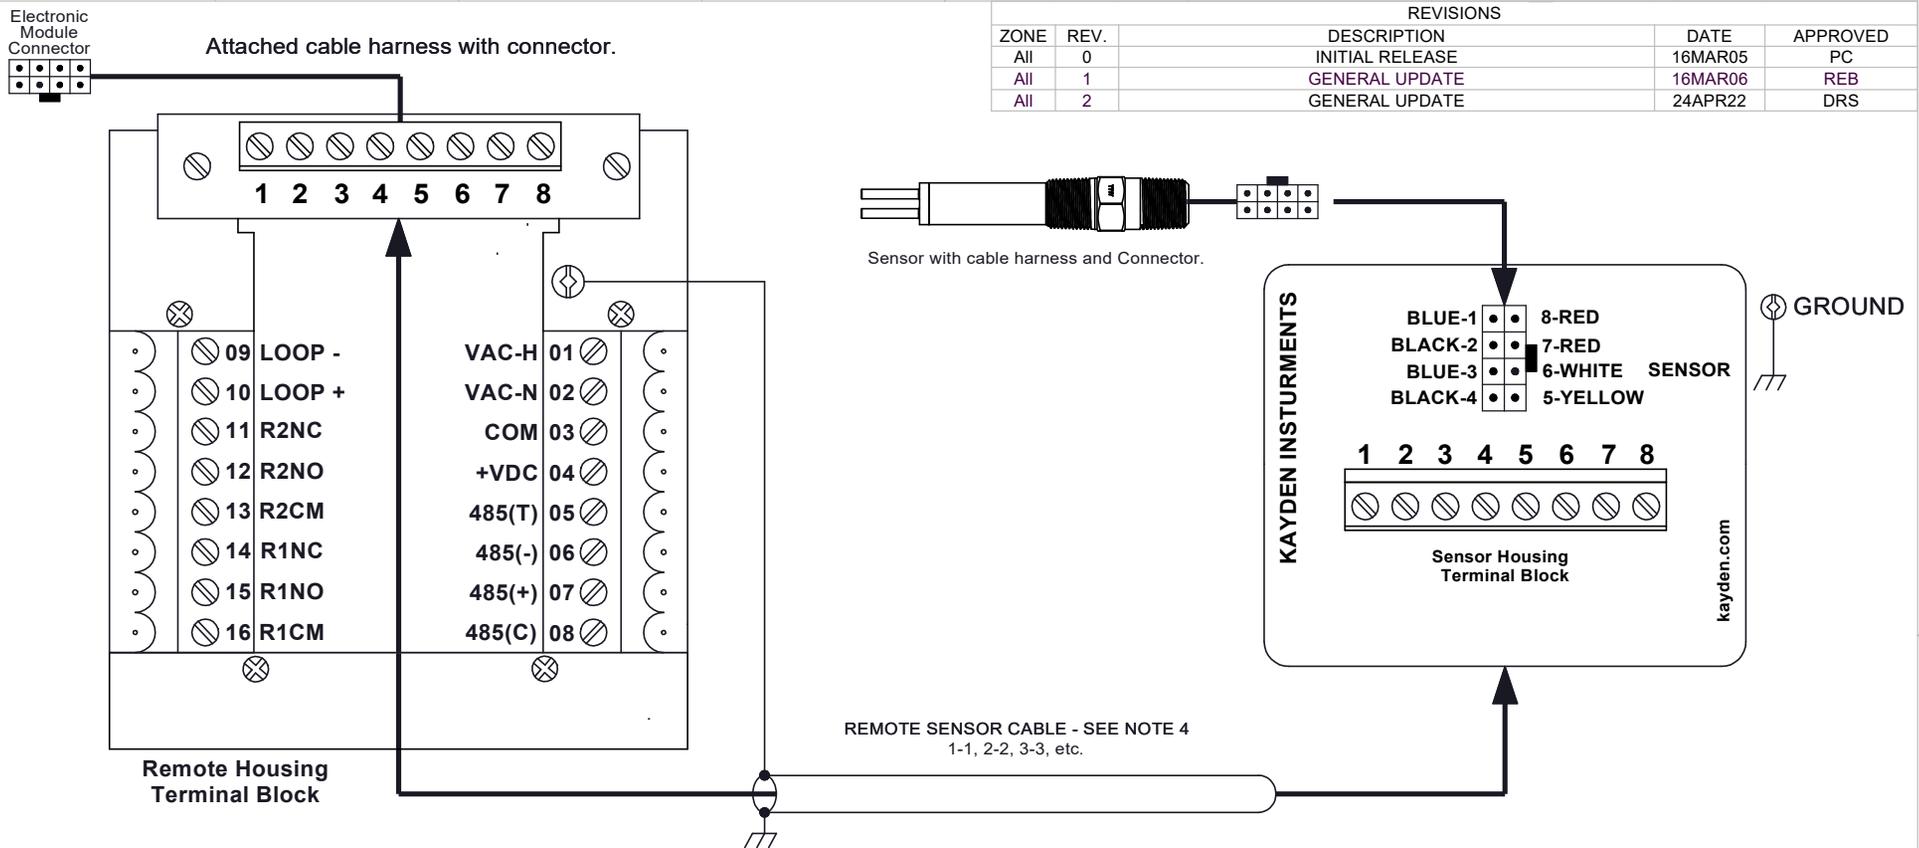

NOTES:

1. This drawing is a reference document only.
2. Colors shown indicate sensor lead wires only. Interconnection wire colors may vary and using wire number labels on the remote cable is recommended.
3. Both Remote Housing and Sensor Housing should be connected to a common low impedance earth ground.
4. Interconnection wires must be 16 to 25 AWG and should have a minimum insulation rating of 600V 90deg C.
5. Remote cable can be ordered from factory if required.

UNLESS OTHERWISE SPECIFIED:	NAME	DATE
DIMENSIONS ARE IN INCHES	DRAWN	READ
TOLERANCES:	CHECKED	MC
ANGULAR: 0.5°	ENG APPR.	PC
ONE PLACE DECIMAL ±0.1		
TWO PLACE DECIMAL ±0.02		
THREE PLACE DECIMAL ±0.007		
INTERPRET GEOMETRIC TOLERANCING PER:		
MATERIAL	COMMENTS:	
FINISH		
DO NOT SCALE DRAWING		



TITLE:		
REMOTE CABLE CONNECTIONS SERIES: CLASSIC		
SIZE	DWG. NO.	REV
B	D15-3001-E	2